



ROTATING RECLINER ARMCHAIR SET

MODEL: ACH-ST-TRON

ASSEMBLY INSTRUCTIONS

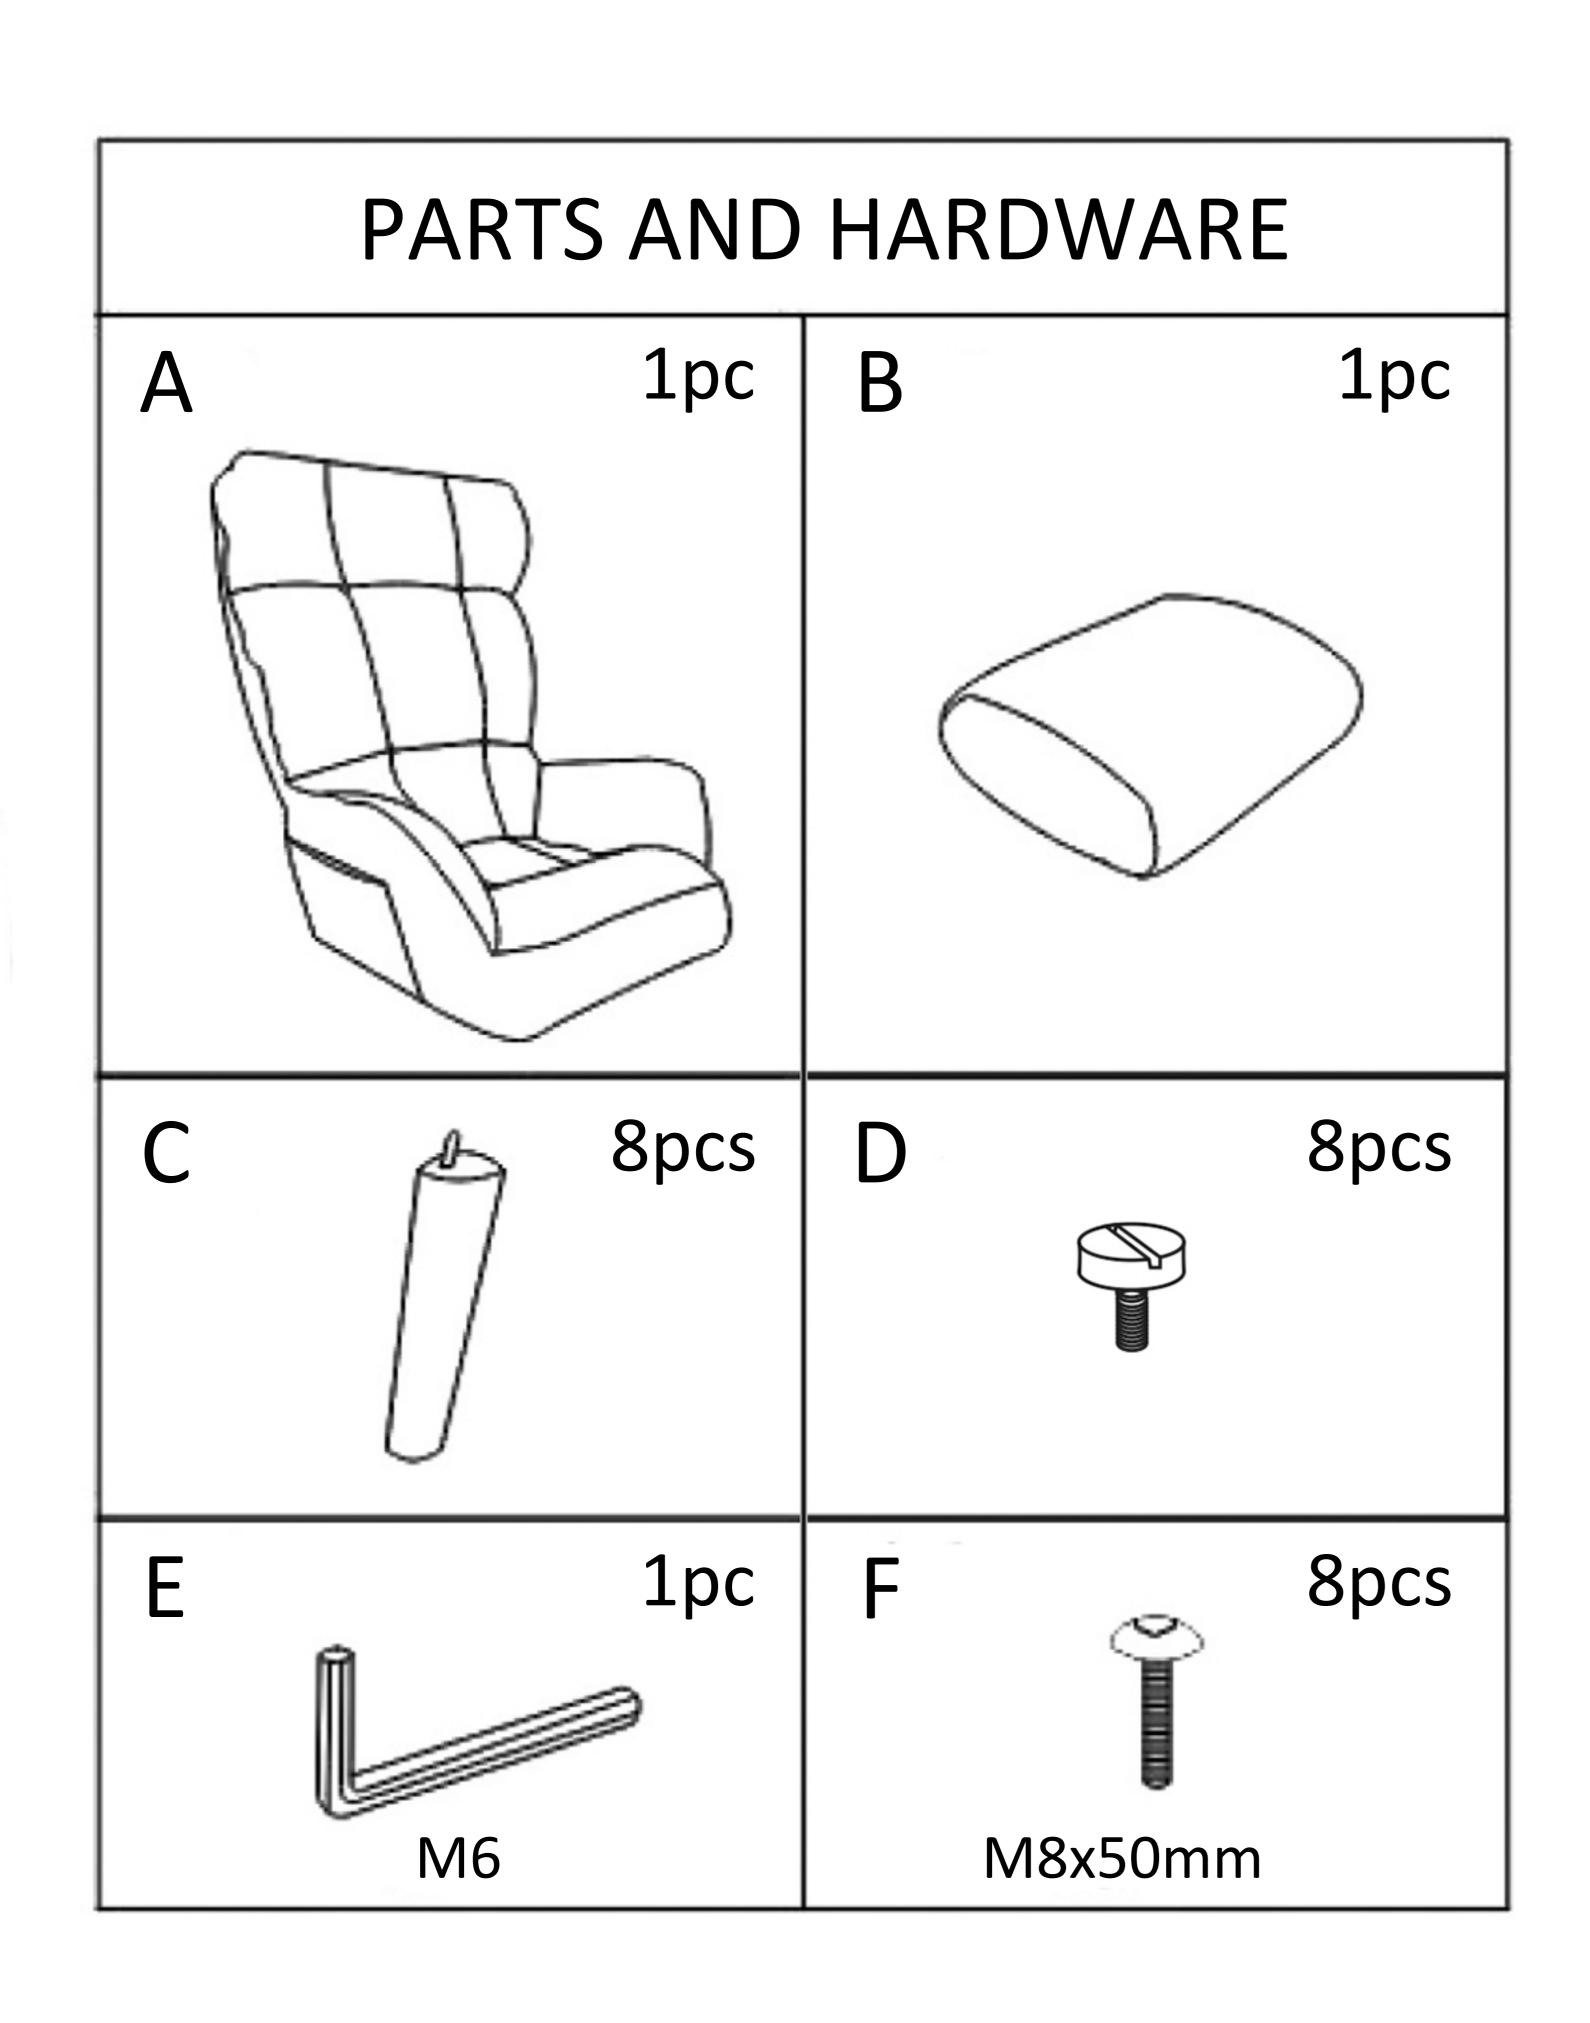

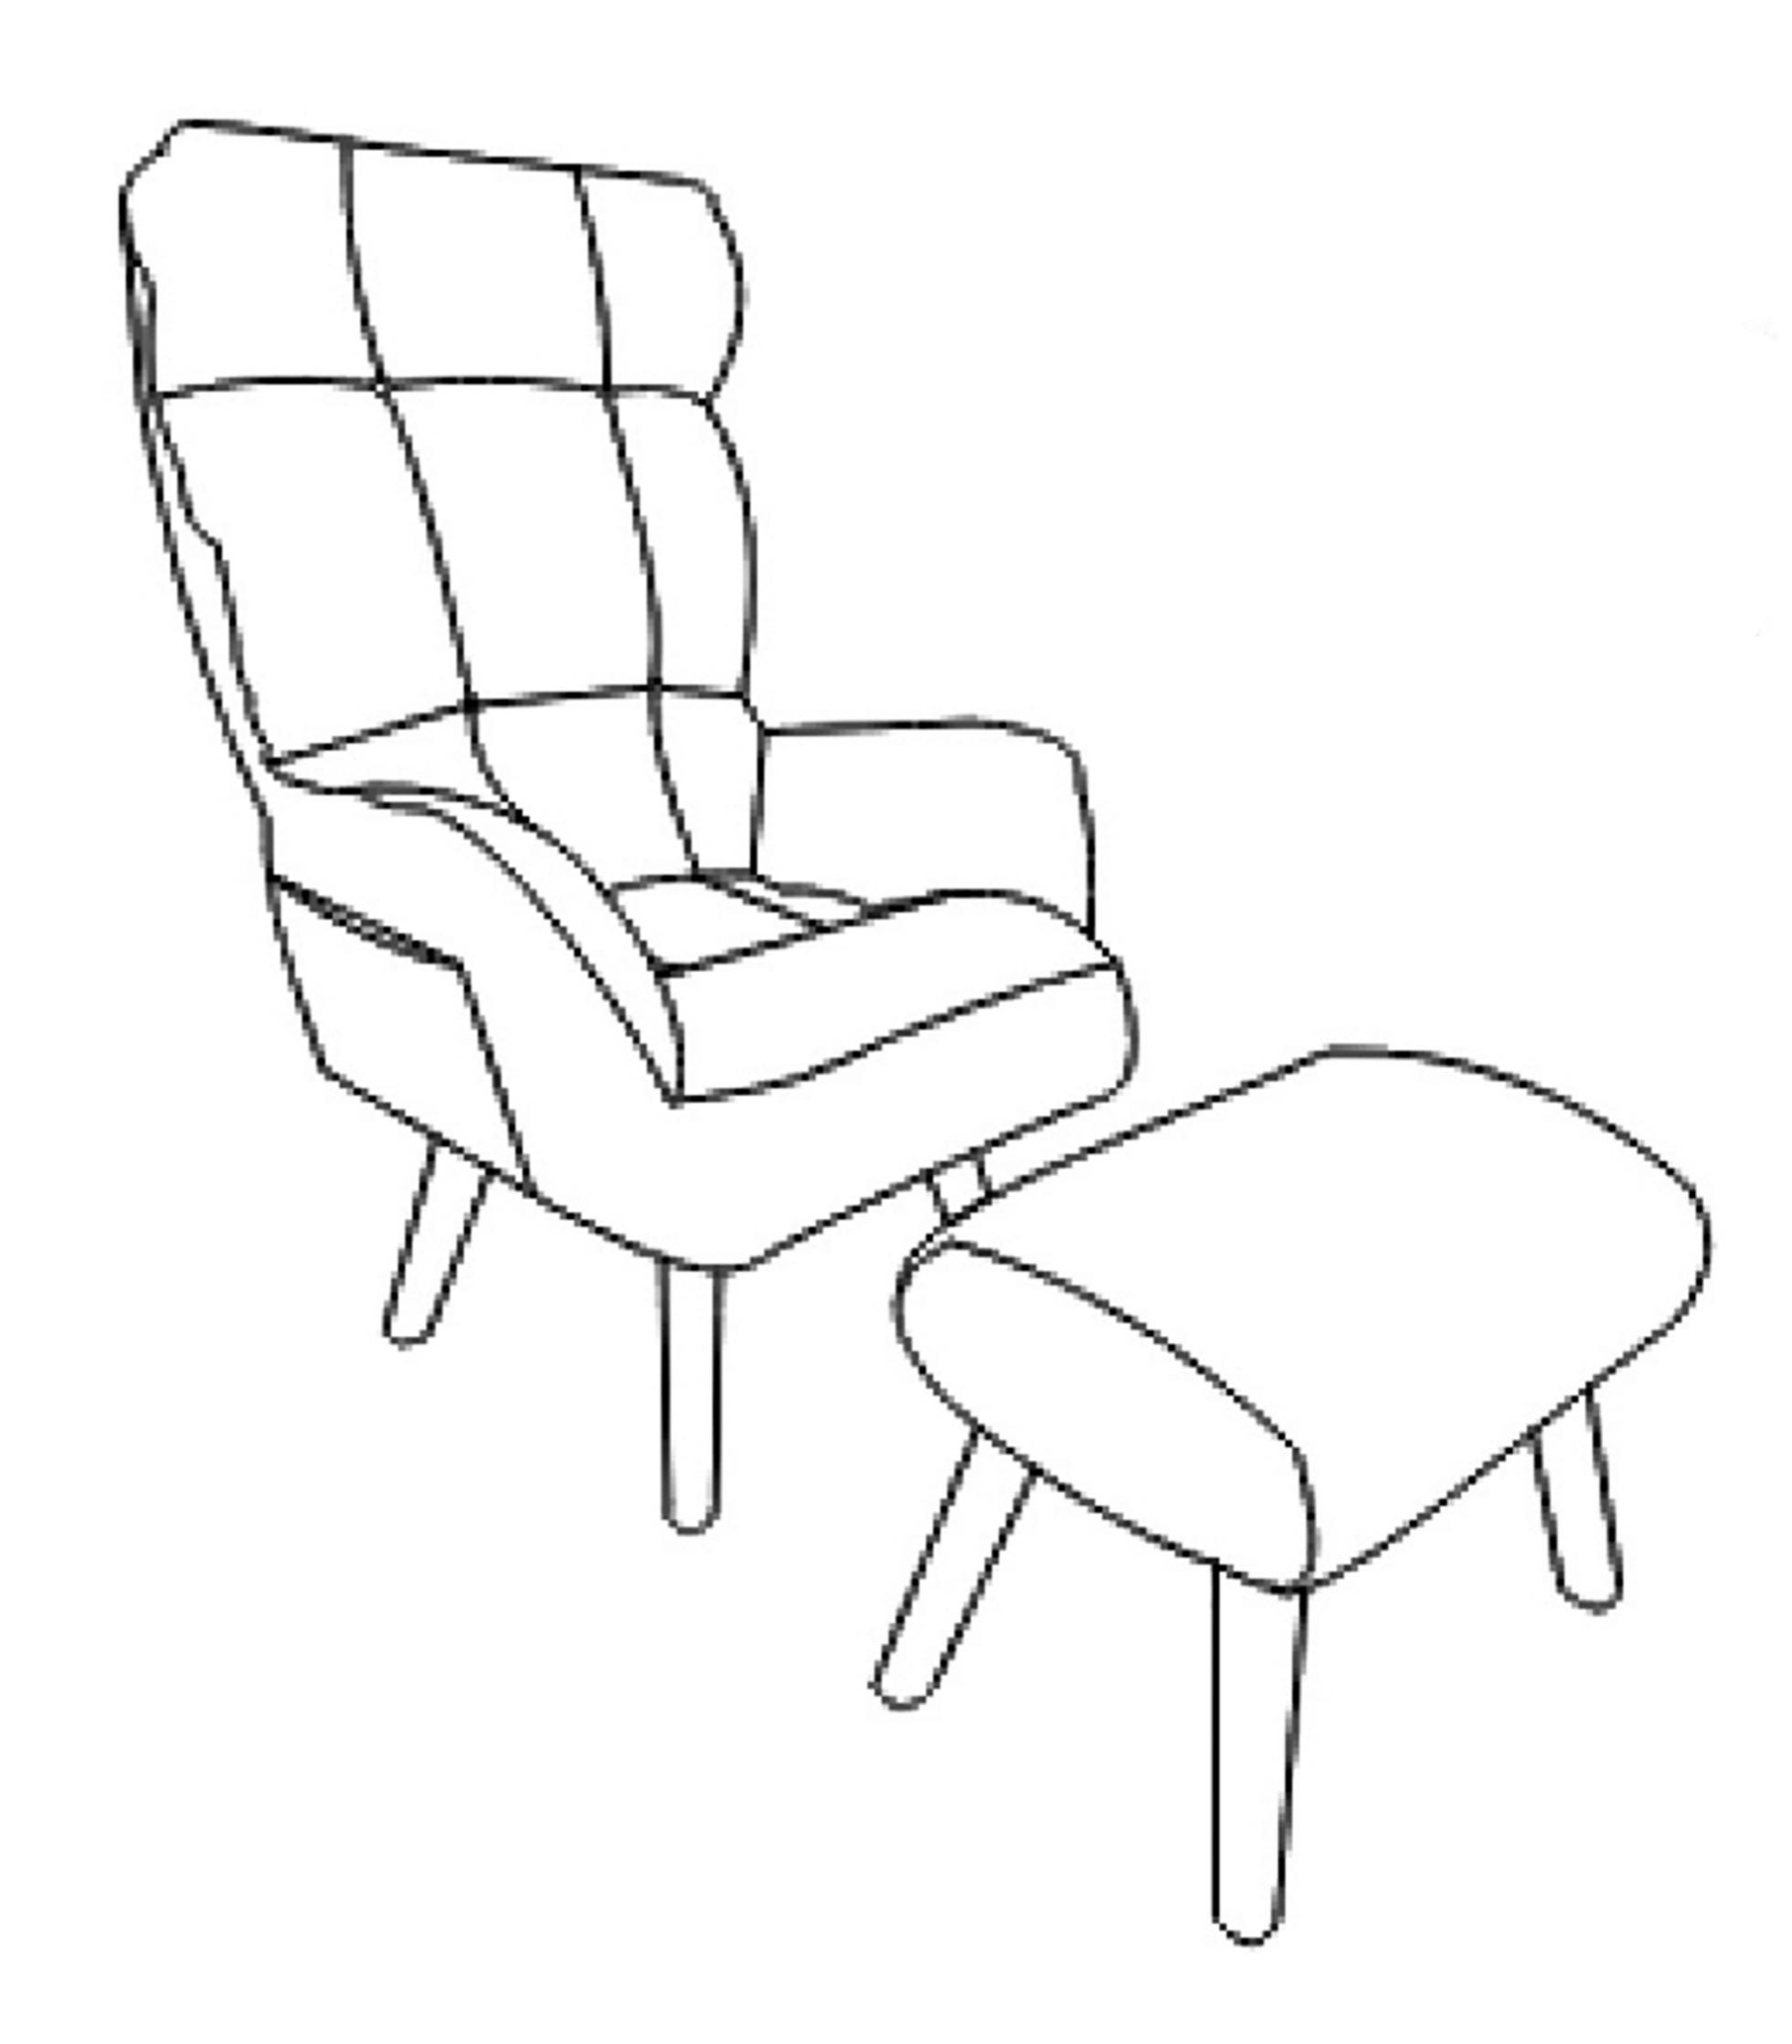


ARMCHAIR ASSEMBLY

FOOTSTOOL ASSEMBLY

E C D F E E

ADJUSTMENTS

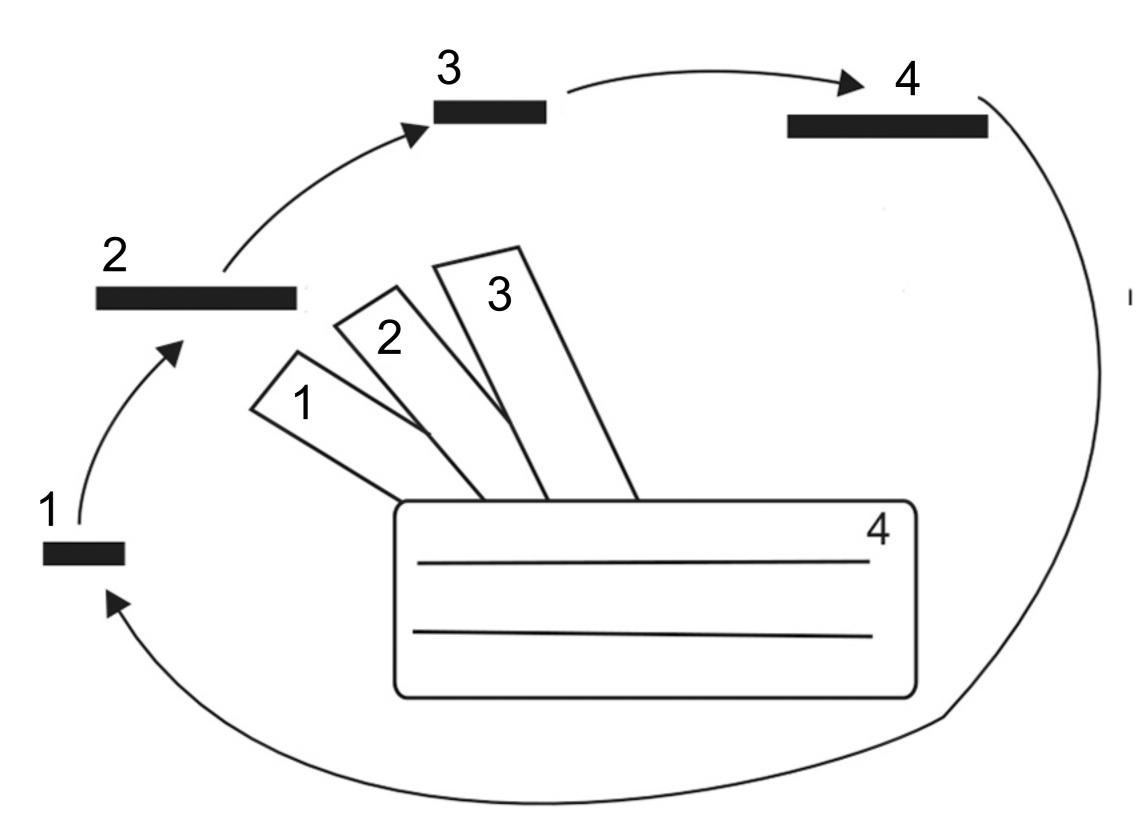

ATTENTION

The adjustment mechanism only works one way forward from Position 1 to 4 and cannot be reclined to previous position directly.

To set Position 1 or 2 from Position 3, please forward the backrest to Position 4 and then start the adjustment from Position 1 again.

WARNING

- 1. Do not stand on the product or use it as a stepping stool.
- 2. Do not use this product until all connections are firmly secured.
- 3. Do not use any sharp tool to open the box or remove the packaging.